



ANNEX F

NOISE



ANNEX F1

CALIBRATION CERTIFICATES FOR NOISE

# *Certificate of Calibration*

*for*

*Description:* **Sound Level Calibrator**

*Manufacturer:* **Larson Davis**

*Type No.:* **CAL 200**

*Serial No.:* **15678**

***Submitted by:***

*Customer:* **Envirotech Services Co.**

*Address:* **Rm. 712, 7/F., My Loft, 9 Hoi Wing Road,**

**Tuen Mun, Hong Kong**

**Upon receipt for calibration, the instrument was found to be:**

☒ **Within**

☐ **Outside**

**the allowable tolerance.**

The test equipments used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

**Date of receipt: 03 January 2025**

**Date of calibration: 06 January 2025**

**Date of NEXT calibration: 05 January 2026**

**Calibrated by:**   
**Calibration Technician**

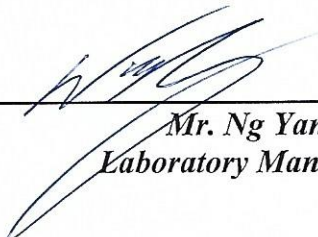**Certified by:**   
**Mr. Ng Yan Wa**  
**Laboratory Manager**

**Date of issue: 06 January 2025**

**Certificate No.: APJ24-124-CC003**



Page 1 of 2

**1. Calibration Precautions:**

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

**2. Calibration Specifications:**

Calibration check

**3. Calibration Conditions:**

Air Temperature: 22.9°C  
Air Pressure: 1019 hPa  
Relative Humidity: 33.2 %

**4. Calibration Equipment:**

Test Equipment	Type	Serial No.	Calibration Report Number	Traceable to
Multifunction Calibrator	B&K 4226	2288467	AV240081	HOKLAS
Sound Level Meter	RION NA-28	30721812	AV240109	HOKLAS

**5. Calibration Results****5.1 Sound Pressure Level**

Nominal value dB	Accept lower level dB	Accept upper level dB	Measured value dB
94.0	93.6	94.4	94.1
114.0	113.6	114.4	114.1

**6. Calibration Results Applied**

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 60942 Class 1.

Note:

The values given in this certification only related to the values measured at the time of the calibration.

Certificate No.: APJ24-124-CC003



Page 2 of 2



# *Certificate of Calibration*

*for*

*Description:* **Sound Level Meter**  
*Manufacturer:* **RION**  
*Type No.:* **NL-52 (Serial No.: 00542913)**  
*Microphone:* **UC-53A (Serial No.: 99995)**  
*Preamplifier:* **NH-25 (Serial No.:43068)**

***Submitted by:***

*Customer:* **Envirotech Services Co.**  
*Address:* **Rm.712, 7/F., My Loft, 9 Hoi Wing Road,  
Tuen Mun, Hong Kong**

**Upon receipt for calibration, the instrument was found to be:**

- ☒ **Within (31.5Hz – 8kHz)**  
☐ **Outside**

**the allowable tolerance.**

The test equipment used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

**Date of receipt: 28 August 2024**

**Date of calibration: 29 August 2024**

**Date of NEXT calibration: 28 August 2025**

**Calibrated by:**   
**Calibration Technician**

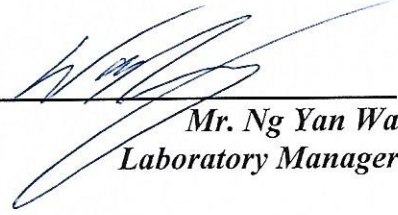**Certified by:**   
**Mr. Ng Yan Wa  
Laboratory Manager**

**Date of issue: 29 August 2024**

**Certificate No.: APJ24-058-CC001**



*Page 1 of 4*

**1. Calibration Precaution:**

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

**2. Calibration Conditions:**

Air Temperature: 24.6 °C  
Air Pressure: 1004 hPa  
Relative Humidity: 53.9 %

**3. Calibration Equipment:**

	Type	Serial No.	Calibration Report Number	Traceable to
Multifunction Calibrator	B&K 4226	2288467	AV240081	HOKLAS

**4. Calibration Results**

Sound Pressure Level

Reference Sound Pressure Level

Setting of Unit-under-test (UUT)				Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting		Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dBA SPL	Fast		94	1000	94.0	±0.4

Linearity

Setting of Unit-under-test (UUT)				Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting		Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dBA SPL	Fast		94	1000	94.0	Ref
				104		104.0	±0.3
				114		114.0	±0.3

Time Weighting

Setting of Unit-under-test (UUT)				Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting		Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dBA SPL	Fast		94	1000	94.0	Ref
		Slow				94.0	±0.3



Certificate No.: APJ24-058-CC001

Page 2 of 4



Frequency Response

Linear Response

Setting of Unit-under-test (UUT)			Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dB	SPL	94	31.5	92.7	$\pm 2.0$
				63	93.7	$\pm 1.5$
				125	93.9	$\pm 1.5$
				250	94.0	$\pm 1.4$
				500	94.0	$\pm 1.4$
				1000	94.0	Ref
				2000	93.9	$\pm 1.6$
				4000	94.3	$\pm 1.6$
				8000	92.4	+2.1; -3.1

A-weighting

Setting of Unit-under-test (UUT)			Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dBA	SPL	94	31.5	53.5	$-39.4 \pm 2.0$
				63	67.5	$-26.2 \pm 1.5$
				125	77.8	$-16.1 \pm 1.5$
				250	85.3	$-8.6 \pm 1.4$
				500	90.8	$-3.2 \pm 1.4$
				1000	94.0	Ref
				2000	95.2	$+1.2 \pm 1.6$
				4000	95.3	$+1.0 \pm 1.6$
				8000	91.3	$-1.1 \pm 2.1$ ; -3.1

C-weighting

Setting of Unit-under-test (UUT)			Applied value		UUT Reading,	IEC 61672 Class 1
Range, dB	Freq. Weighting	Time Weighting	Level, dB	Frequency, Hz	dB	Specification, dB
30-130	dBC	SPL	94	31.5	89.7	$-3.0 \pm 2.0$
				63	92.9	$-0.8 \pm 1.5$
				125	93.8	$-0.2 \pm 1.5$
				250	94.0	$-0.0 \pm 1.4$
				500	94.0	$-0.0 \pm 1.4$
				1000	94.0	Ref
				2000	93.8	$-0.2 \pm 1.6$
				4000	93.5	$-0.8 \pm 1.6$
				8000	89.4	$-3.0 \pm 2.1$ ; -3.1



Certificate No.: APJ24-058-CC001

Page 3 of 4

## 5. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

94 dB	31.5 Hz	± 0.10
	63 Hz	± 0.10
	125 Hz	± 0.10
	250 Hz	± 0.10
	500 Hz	± 0.10
	1000 Hz	± 0.05
	2000 Hz	± 0.05
	4000 Hz	± 0.10
	8000 Hz	± 0.10
104 dB	1000 Hz	± 0.05
114 dB	1000 Hz	± 0.05

The uncertainties are evaluated for a 95% confidence level.

### Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)\*L shall not be liable for any loss or damage resulting from the use of the equipment.





ANNEX F2

MONITORING SCHEDULE FOR NOISE

**Tung Chung New Town Extension (East)**  
**Noise Monitoring Schedule (July 2025)**

Sunday	Monday	Tuesday	Wednesday	Thursday	Friday	Saturday
		1-Jul	2-Jul	3-Jul	4-Jul	5-Jul
						Noise Monitoring
6-Jul	7-Jul	8-Jul	9-Jul	10-Jul	11-Jul	12-Jul
					Noise Monitoring	
13-Jul	14-Jul	15-Jul	16-Jul	17-Jul	18-Jul	19-Jul
				Noise Monitoring		
20-Jul	21-Jul	22-Jul	23-Jul	24-Jul	25-Jul	26-Jul
			Noise Monitoring			
27-Jul	28-Jul	29-Jul	30-Jul	31-Jul		
		Noise Monitoring				



ANNEX F3


MONITORING RESULTS FOR NOISE



**Table F3.1 Data for Noise Monitoring at Station NMS-CA-1A during Normal Working Hours (0700-1900 hours)**

Date & Time	L <sub>eq</sub> (5min)	L <sub>10</sub>	L <sub>90</sub>	L <sub>eq</sub> (30min)
7/5/2025 9:37	66.1	68.0	61.3	66.4
7/5/2025 9:42	66.8	68.6	60.4	
7/5/2025 9:47	64.5	67.7	59.3	
7/5/2025 9:52	67.9	70.2	59.5	
7/5/2025 9:57	67.0	68.8	60.7	
7/5/2025 10:02	65.4	68.0	60.7	66.2
7/11/2025 9:40	66.9	70.6	59.6	
7/11/2025 9:45	67.0	68.4	58.7	
7/11/2025 9:50	66.1	69.9	59.1	
7/11/2025 9:55	66.3	69.4	59.2	
7/11/2025 10:00	64.8	67.2	60.3	
7/11/2025 10:05	65.6	67.9	59.5	65.3
7/17/2025 15:09	65.2	68.0	59.7	
7/17/2025 15:14	62.7	65.9	58.2	
7/17/2025 15:19	64.3	66.3	58.1	
7/17/2025 15:24	66.2	66.6	58.0	
7/17/2025 15:29	68.0	71.3	62.1	
7/17/2025 15:34	63.0	66.1	58.3	66.8
7/23/2025 9:37	69.4	71.7	60.2	
7/23/2025 9:42	67.4	70.4	60.1	
7/23/2025 9:47	67.8	68.4	60.6	
7/23/2025 9:52	65.1	67.4	60.9	
7/23/2025 9:57	64.0	66.6	60.7	
7/23/2025 10:02	64.4	66.8	60.8	66.8
7/29/2025 11:39	66.9	67.3	58.9	
7/29/2025 11:44	65.1	68.3	60.3	
7/29/2025 11:49	69.1	70.0	60.5	
7/29/2025 11:54	62.9	65.6	59.6	
7/29/2025 11:59	63.7	66.6	59.0	
7/29/2025 12:04	69.1	71.6	59.3	


**Figure F3.1 Graphical Presentation for Noise Monitoring at Station NMS-CA-1A**

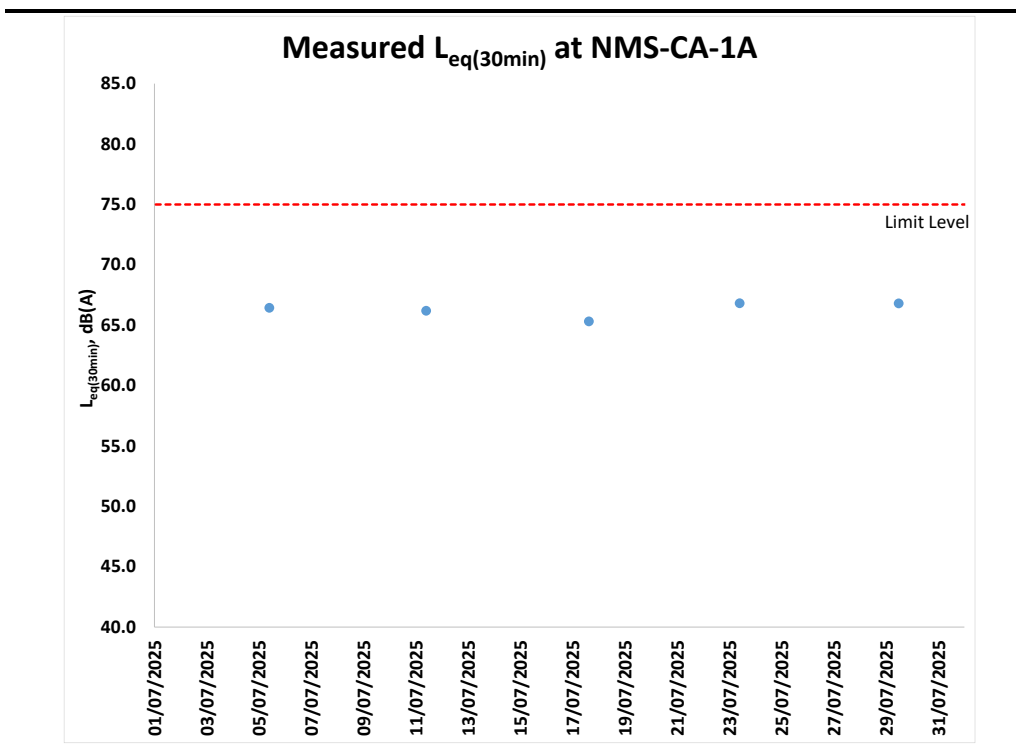

**Table F3.2 Data for Noise Monitoring at Station NMS-CA-4 during Normal Working Hours (0700-1900 hours)**

Date & Time	L <sub>eq</sub> (5min)	L <sub>10</sub>	L <sub>90</sub>	L <sub>eq</sub> (30min)
7/5/2025 9:01	63.7	64.7	62.7	64.5
7/5/2025 9:06	63.9	65.2	62.5	
7/5/2025 9:11	64.3	65.4	62.9	
7/5/2025 9:16	65.0	66.5	63.0	
7/5/2025 9:21	64.5	65.4	63.5	
7/5/2025 9:26	65.2	66.2	63.7	67.2
7/11/2025 9:00	65.8	67.1	64.3	
7/11/2025 9:05	66.3	67.1	64.9	
7/11/2025 9:10	68.2	69.8	64.8	
7/11/2025 9:15	68.1	70.0	64.7	
7/11/2025 9:20	67.8	70.0	65.6	66.5
7/11/2025 9:25	66.2	67.0	65.2	
7/17/2025 14:34	67.2	69.5	61.7	
7/17/2025 14:39	66.0	68.5	61.4	
7/17/2025 14:44	66.5	69.3	61.2	
7/17/2025 14:49	66.7	69.6	60.6	67.6
7/17/2025 14:54	67.0	69.3	61.7	
7/17/2025 14:59	65.1	67.8	59.6	
7/23/2025 9:01	66.9	67.9	64.8	
7/23/2025 9:06	66.9	68.3	65.2	
7/23/2025 9:11	68.2	69.9	66.0	62.5
7/23/2025 9:16	66.5	67.7	64.6	
7/23/2025 9:21	67.4	68.6	65.3	
7/23/2025 9:26	69.2	70.8	66.2	
7/29/2025 11:04	61.9	63.4	60.4	
7/29/2025 11:09	62.0	63.2	60.7	62.5
7/29/2025 11:14	63.5	64.8	62.2	
7/29/2025 11:19	62.6	63.8	61.1	
7/29/2025 11:24	62.5	63.8	61.1	
7/29/2025 11:29	62.3	63.7	60.9	

**Figure F3.2 Graphical Presentation for Noise Monitoring at Station NMS-CA-4**

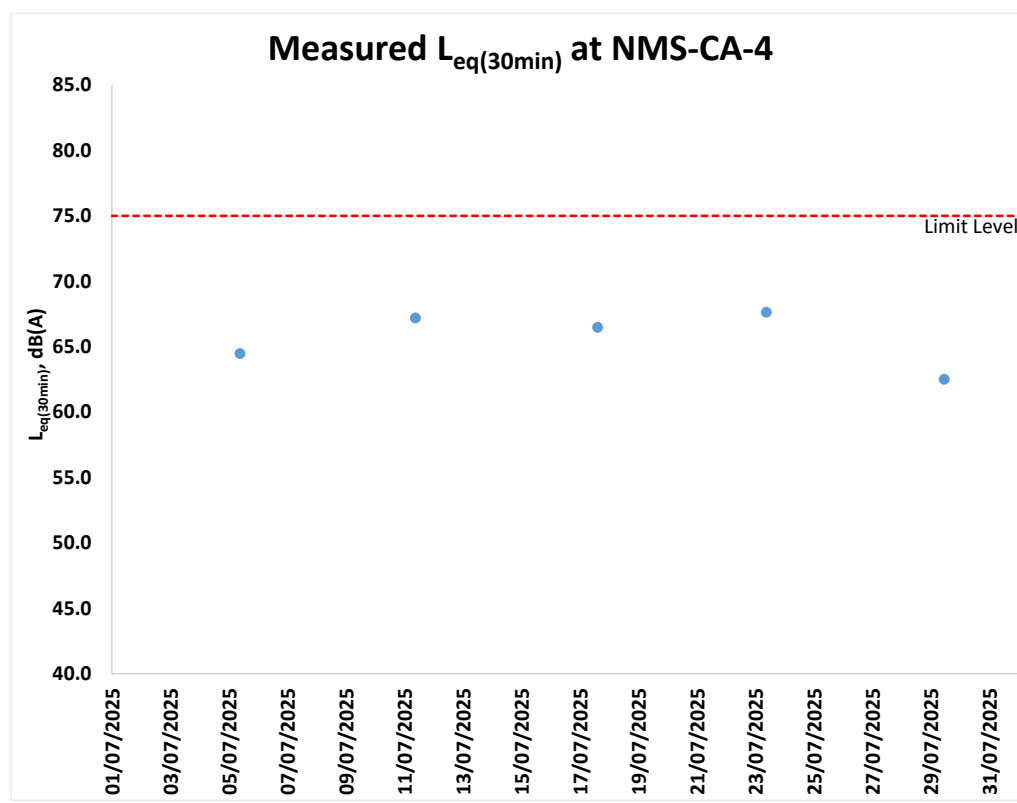



ANNEX F4

EVENT AND ACTION PLAN FOR NOISE



**Annex F4**      **Event and Action Plan for Construction Noise**

Event	Action			
	ET	IEC	ER	Contractor
Action Level Exceedance	<ol style="list-style-type: none"> <li>1. Notify IEC, ER and Contractor;</li> <li>2. Carry out investigation;</li> <li>3. Report the results of investigation to the IEC, ER and Contractor;</li> <li>4. Discuss with the Contractor and formulate remedial measures;</li> <li>5. Increase monitoring frequency to check mitigation effectiveness.</li> </ol>	<ol style="list-style-type: none"> <li>1. Review the analysed results submitted by the ET;</li> <li>2. Review the proposed remedial measures by the Contractor and advise the ER accordingly;</li> <li>3. Supervise the implementation of remedial measures.</li> </ol>	<ol style="list-style-type: none"> <li>1. Confirm receipt of notification of failure in writing;</li> <li>2. Notify Contractor;</li> <li>3. Require Contractor to propose remedial measures for the analysed noise problem;</li> <li>4. Ensure remedial measures are properly implemented</li> </ol>	<ol style="list-style-type: none"> <li>1. Submit noise mitigation proposals to IEC and ER;</li> <li>2. Implement noise mitigation proposals.</li> </ol>
Limit Level Exceedance	<ol style="list-style-type: none"> <li>1. Identify source;</li> <li>2. Inform IEC, ER, EPD and Contractor;</li> <li>3. Repeat measurements to confirm findings;</li> <li>4. Increase monitoring frequency;</li> <li>5. Carry out analysis of Contractor's working procedures to determine possible mitigation to be implemented;</li> <li>6. Inform IEC, ER and EPD the causes and actions taken for the exceedances;</li> <li>7. Assess effectiveness of Contractor's remedial actions and keep IEC, EPD and ER informed of the results;</li> <li>8. If exceedance stops, cease additional monitoring.</li> </ol>	<ol style="list-style-type: none"> <li>1. Discuss amongst ER, ET, and Contractor on the potential remedial actions;</li> <li>2. Review Contractors remedial actions whenever necessary to assure their effectiveness and advise the ER accordingly;</li> <li>3. Supervise the implementation of remedial measures.</li> </ol>	<ol style="list-style-type: none"> <li>1. Confirm receipt of notification of failure in writing;</li> <li>2. Notify Contractor;</li> <li>3. Require Contractor to propose remedial measures for the analysed noise problem;</li> <li>4. Ensure remedial measures properly implemented;</li> <li>5. If exceedance continues, consider what portion of the work is responsible and instruct the Contractor to stop that portion of work until the exceedance is abated.</li> </ol>	<ol style="list-style-type: none"> <li>1. Take immediate action to avoid further exceedance;</li> <li>2. Submit proposals for remedial actions to IEC within 3 working days of notification;</li> <li>3. Implement the agreed proposals;</li> <li>4. Resubmit proposals if problem still not under control;</li> <li>5. Stop the relevant portion of works as determined by the ER until the exceedance is abated.</li> </ol>